



Regeneration  
by Design

# RegenerOss<sup>®</sup>

Allograft



 **ZimVie**



# RegenerOss

## Allograft

### Safety You Can Build On

RegenerOss Allograft\* can alleviate the need for a second operative site when faced with inadequate autogenous bone size, shape, or volume, thus preventing increased post-operative pain and donor site morbidity. In addition, studies have shown that allograft bone can produce osseogenesis by activating mesenchymal cells to form bone.<sup>1</sup>

**RegenerOss Allograft can be utilized in a variety of dental applications, either by itself or as a graft extender. The following are common sites for allograft tissue use:**

- Extraction socket preservation
- Ridge augmentation and reconstruction
- Peri-implant defects
- Sinus floor elevation

EASY TO OPEN

DAPPEN-DISH STYLE  
CONTAINER CAN BE  
USED FOR HYDRATING  
PRODUCT




\* RegenerOss Allograft Particulate products are distributed by ZimVie Dental and processed by Community Tissue Services. Prior to August, 2016, distinct lots of RegenerOss Allograft Particulate products were processed by University of Miami Tissue Bank (UMTB). Orders may be fulfilled with product originating from either or both tissue establishment until depletion of UMTB stock.

1. Misch CE, Dietsch F. Bone-grafting materials in implant dentistry. *Implant Dent.* 1993 Fall;2(3):158-67.

## Steps for Enhanced Safety

For site development, RegenerOss Allograft is the allograft of choice. Derived from a single source for increased protection against cross-contamination, RegenerOss Allograft Bone is:

- Aseptically processed tissue for better regenerative properties and safety without destruction of the tissue
- Utilizing a proprietary processing technique that removes unwanted cells, yet preserves valuable lipids
- Available in a broad range of configurations for regenerating a variety of challenging sites
- Single-source service from donor screening and selection to tissue recovery and processing for increased protection against cross-contamination
- All tissues undergo various quality checks prior to release
- All tissues are processed in class 100 (certified) clean rooms
- All test reports are reviewed by a medical director for approval before tissue is released

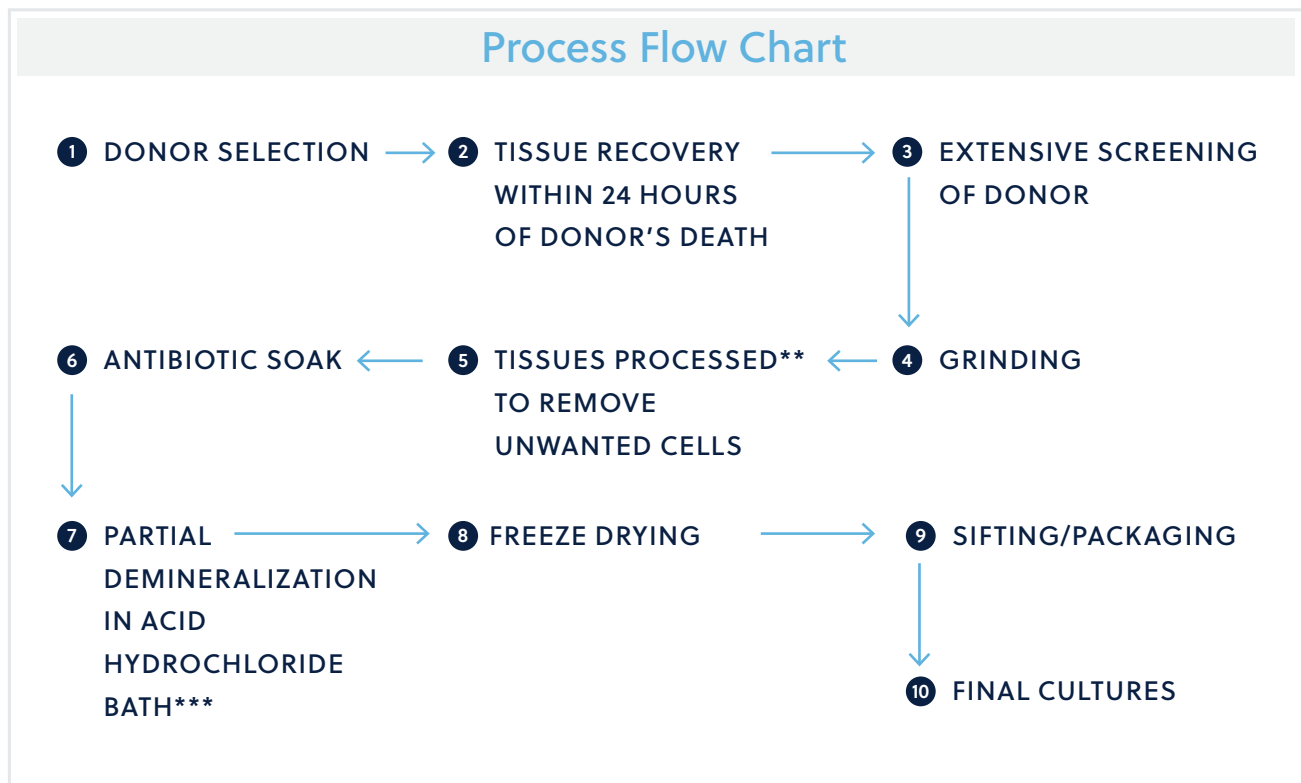

\*\* In all forms, the majority of the fat is washed away using warm sterile water, not harsh chemicals, to protect the Bone Morphogenetic Proteins (BMP)

\*\*\* Demineralized tissues only

# RegenerOss Allograft Ordering Information

Mineralized		
Item Numbers	Particle Size	Description
RMCA205	200-300 µm	Cancellous, Mineralized, 0.5 cc
RMCA210	200-300 µm	Cancellous, Mineralized, 1.0 cc
RMCA220	200-300 µm	Cancellous, Mineralized, 2.0 cc
RMCA305	300-500 µm	Cancellous, Mineralized, 0.5 cc
RMCA310	300-500 µm	Cancellous, Mineralized, 1.0 cc
RMCA320	300-500 µm	Cancellous, Mineralized, 2.0 cc
RMCA505	500-800 µm	Cancellous, Mineralized, 0.5 cc
RMCA510	500-800 µm	Cancellous, Mineralized, 1.0 cc
RMCA520	500-800 µm	Cancellous, Mineralized, 2.0 cc

Mineralized		
Item Numbers	Particle Size	Description
RMCO205	200-300 µm	Cortical, Mineralized, 0.5 cc
RMCO210	200-300 µm	Cortical, Mineralized, 1.0 cc
RMCO220	200-300 µm	Cortical, Mineralized, 2.0 cc
RMCO305	300-500 µm	Cortical, Mineralized, 0.5 cc
RMCO310	300-500 µm	Cortical, Mineralized, 1.0 cc
RMCO320	300-500 µm	Cortical, Mineralized, 2.0 cc
RMCO505	500-800 µm	Cortical, Mineralized, 0.5 cc
RMCO510	500-800 µm	Cortical, Mineralized, 1.0 cc
RMCO520	500-800 µm	Cortical, Mineralized, 2.0 cc

Demineralized		
Item Numbers	Particle Size	Description
RDCO205	200-300 µm	Cortical, Part. Demineralized, 0.5 cc
RDCO210	200-300 µm	Cortical, Part. Demineralized, 1.0 cc
RDCO220	200-300 µm	Cortical, Part. Demineralized, 2.0 cc
RDCO305	300-500 µm	Cortical, Part. Demineralized, 0.5 cc
RDCO310	300-500 µm	Cortical, Part. Demineralized, 1.0 cc
RDCO320	300-500 µm	Cortical, Part. Demineralized, 2.0 cc
RDCO505	500-800 µm	Cortical, Part. Demineralized, 0.5 cc
RDCO510	500-800 µm	Cortical, Part. Demineralized, 1.0 cc
RDCO520	500-800 µm	Cortical, Part. Demineralized, 2.0 cc



Scan for IFU

For more information visit [ZimVie.com](http://ZimVie.com)

ZimVie  
4555 Riverside Drive  
Palm Beach Gardens, FL 33410  
Phone: +1-561-776-6700  
Fax: +1-561-776-1272



Unless otherwise indicated, as referenced herein, all trademarks are the property of ZimVie; and all products are manufactured by one or more of the dental subsidiaries of ZimVie Inc. (Biomet 3i, LLC, Zimmer Dental Inc., etc.) and marketed and distributed by ZimVie Dental (formerly Zimmer Biomet Dental) and its authorized marketing partners. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians use only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of ZimVie. ZV1547 REV A 08/23 ©2023 ZimVie. All rights reserved.

